

	DOCUMENT NO:	CDS- L612nn-06XX-YYYYZZ- EVO	VER:	1.1
	Liquid 6 EVO Cartridge, Thermoplastic			EFFECTIVE DATE:
APPROVAL:	ECO-273	Jupiter PN(s):	See part number legend	PAGE 1 OF 4

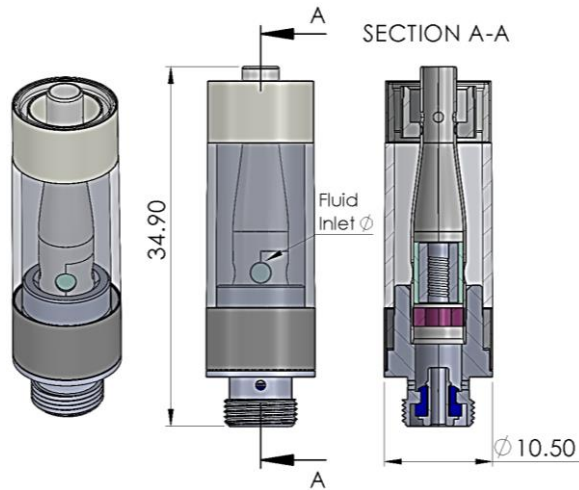

0.5ml

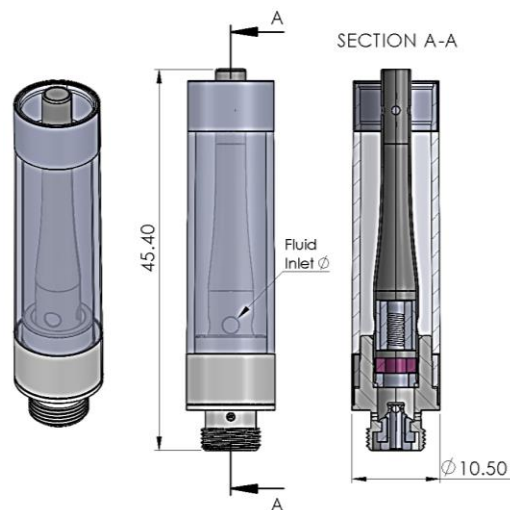


1.0ml

Description: Top fill vaporizer cartridge


Features:

- CCELL Technology atomizer – heating element embedded in porous ceramic
- Tamper proof press-fit mouthpiece - standard mouthpiece options listed in *L6 ETP Mouthpiece CDS*
- 510 connection – M7 threaded connection
- Operational viscosity ranges from 1,000 - 700,000 cPs @ 25°C [77°F]

	DOCUMENT NO:	CDS- L612nn-06XX-YYYYZZZ-EVO	VER:	1.1
	Liquid 6 EVO Cartridge, Thermoplastic			EFFECTIVE DATE:
APPROVAL:	ECO-273	Jupiter PN(s):	See part number legend	PAGE 2 OF 4

- Available in varying powers and fluid inlet sizes to customize vapor feel and taste

Specifications		
Version (size)	0.5 ml	1.0 ml
Max. fill volume	0.50 ml	1.00 ml
Weight, empty	6.1g	6.6g
Power		
Standard power is 9W; Other options available upon request.		
Fluid Inlet Diameter		
Standard inlet diameter is 2.0mm; See part number legend for other options.		
Number of Inlets		
2x for 2.6mm inlet diameter 4x for 2.0mm and 2.3 mm inlet diameter		
Viscosity Range		
1,000 - 700,000 cPs @ 25°C [77°F]		
Wetted Materials		
Fluid Housing	Eng. Thermoplastic (proprietary)	
Sleeves	Stainless Steel (SS)	
Airway tube & Heater base	Stainless Steel (SS)	
Heating element	Nichrome	
Wick	CCELL EVO Ceramic	
Atomizer retaining wrap	Cellulose	
Seals	Silicone	
Branding Options		
Available with MOQ		
Recommended Operating Conditions		
Working Temperature:	-10°C to 60°C	Working Humidity:
		35% - 70%
Recommended Storage Conditions		
Storage Temperature:	23°C – 28°C	Storage Humidity:
		35% - 70%
Recommended Assembly force		
220lbs		
Safety Certifications		
<ul style="list-style-type: none"> • RoHS 		

jupiter 	DOCUMENT NO:	CDS- L612nn-06XX-YYYYZZZ-EVO	VER:	1.1
	Liquid 6 EVO Cartridge, Thermoplastic			EFFECTIVE DATE:
APPROVAL:	ECO-273	Jupiter PN(s):	See part number legend	PAGE 3 OF 4

Part Number Legend – L612nn-06XX*-YYYYZZZ-EVO		
<ul style="list-style-type: none"> • nn -> Cartridge Volume <ul style="list-style-type: none"> ○ 05 for 0.5g ○ 10 for 1.0g 	<ul style="list-style-type: none"> • YYY -> Cartridge Power <ul style="list-style-type: none"> ○ 009 for 9W (1.4ohm) ○ 007 for 7W (1.7ohm) ○ 016 for 6W (1.9ohm) 	<ul style="list-style-type: none"> • ZZZ -> Fluid Inlet Dia. <ul style="list-style-type: none"> ○ 002 for 2.0mm ○ 203 for 2.3mm ○ 206 for 2.6mm

*XX digits denote product branding

Liquid 6, EVO ETP Cartridge with Stainless Steel Airway Filling Instructions


Failure to follow these instructions may result in cartridge leakage or poor performance.

Jupiter Liquid 6, ETP EVO Cartridges with Stainless Steel Airways (SSA) are top-fill cartridges available in 0.5, 1.0ml versions. The two versions differ only in the length of the reservoir. If you are unsure which version you have, measure the length without the mouthpiece. Refer to the drawing on page 1 to determine where to measure and which cartridge you have.

Multiple mouthpiece styles are available. All press on in the same manner.

Filling Instructions


1. Insert a blunt tipped needle (14 ga. or smaller) into the space between the airway and the outer wall of the cartridge (see the image, below).

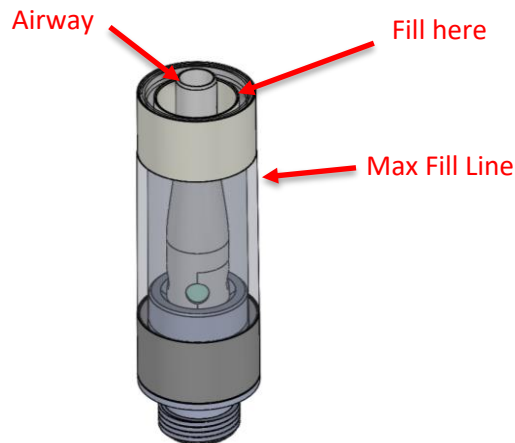

While the cartridge is oriented vertically with the threaded connector downward, fill the cartridge through the needle. Do not overfill.

Caution: Do not allow fluid to enter the airway (center tube).

2. Immediately after filling, insert and press-fit the mouthpiece until it is fully seated. Mechanical assistance, such as an arbor press or channel lock pliers, is required to fully seat the mouthpiece.

		DOCUMENT NO:	CDS- L612nn-06XX-YYYYZZ- EVO	VER:	1.1
		Liquid 6 EVO Cartridge, Thermoplastic			EFFECTIVE DATE:
APPROVAL:	ECO-273	Jupiter PN(s):	See part number legend	PAGE 4 OF 4	

220lbs of force is recommended to close the cartridges. Damage to the cartridge can be caused when forces are above 400lbf.

Caution: Failure to install the mouthpiece within 2 minutes of filling may result in leakage.

- Cartridges should be allowed to stand for at least 30 minutes before use to allow the atomizer to saturate and create headspace. The rate that the atomizer saturates is dependent upon the viscosity of the fluid. More viscous fluids may require more time.

Caution: If cleaning the cartridge housing after filling and capping, use a diluted solution of <70% alcohol to avoid fogging

Caution: Jupiter cartridges are disposable and for single use only. Do not refill or use Jupiter cartridges with tobacco derived products.

- If the cartridge/device is to experience a pressure change because of an increase in temperature or a change in elevation, the cartridge/device must be shipped with the MP facing down, allowing for the inlets to be exposed to ambient air.

For Technical Assistance please contact us at: CS@JupiterResearch.com