

		DOCUMENT NO:	CDS-L612nn-50XX-YYYYZZ-EVO	VER:	1.1
		Liquid 6 EVO Cartridge, Glass Screw-on			EFFECTIVE DATE: 1/27/2023
APPROVAL:	ECO-273	Jupiter PN(s):	See part number legend	PAGE 1 OF 4	

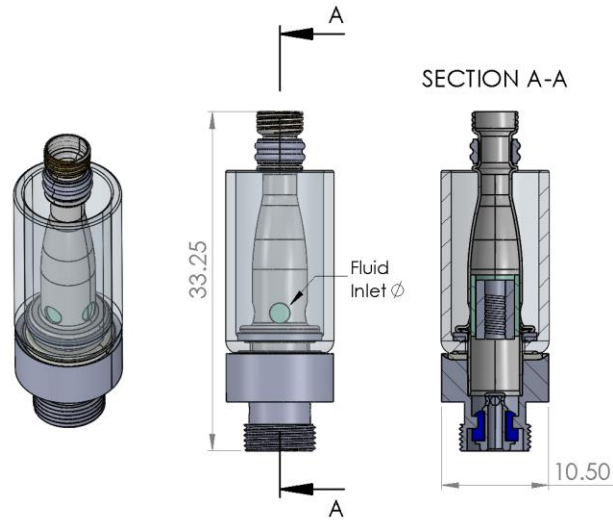

0.5ml

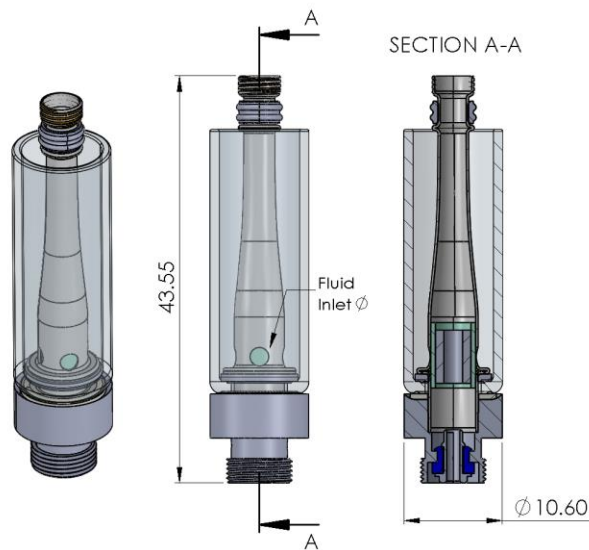


1.0ml

Description: Top fill vaporizer cartridge


Features:

- CCELL Technology atomizer – heating element embedded in porous ceramic
- Screwed mouthpiece - standard mouthpiece options listed in *L6 Glass Screw-on EVO Mouthpiece CDS*

	DOCUMENT NO:	CDS-L612nn-50XX-YYYYZZZ-EVO	VER:	1.1
	Liquid 6 EVO Cartridge, Glass Screw-on			EFFECTIVE DATE: 1/27/2023
APPROVAL:	ECO-273	Jupiter PN(s):	See part number legend	PAGE 2 OF 4

- 510 connection – M7 threaded connection
- Operational viscosity ranges from 1,000 - 700,000 cPs @ 25°C [77°F]
- Available in varying powers and fluid inlet sizes to customize vapor feel and taste

Specifications		
Version (size)	0.5 ml	1.0 ml
Internal Volume (Gross)	0.55 ml	1.05 ml
Max. Fill Volume	0.50 ml	1.00 ml
Weight, empty	5.3g	6.4g
Power		
Standard power is 9W; Other options available upon request		
Fluid Inlet Diameter		
Standard inlet diameter is 2.0mm; See part number legend for other options.		
Number of inlets		
2x for 2.6mm inlet diameter 4x for 2.0mm and 2.3mm inlet diameter		
Viscosity Range		
1,000 - 700,000 cPs		
Recommended closing torque		
4.0kgf*cm [3.5lbf*in]		
Wetted Materials		
Fluid Housing	Glass	
Atomizer shell & Airway tube	Stainless Steel (SS)	
Heating element	Nichrome	
Wick	CCELL EVO Ceramic	
Atomizer retaining wrap	Cellulose	
Seals	Silicone	
Branding Options		
Available with MOQ		
Part Number Legend – L612nn-50XX-YYYYZZZ-EVO		
<ul style="list-style-type: none"> • nn -> Cartridge Volume <ul style="list-style-type: none"> ○ 05 for 0.5g ○ 10 for 1.0g 	<ul style="list-style-type: none"> • YYY -> Cartridge Power <ul style="list-style-type: none"> ○ 009 for 9W (1.4ohm) ○ 007 for 7W (1.7ohm) ○ 016 for 6W (1.9ohm) 	<ul style="list-style-type: none"> • ZZZ -> Fluid Inlet Dia. <ul style="list-style-type: none"> ○ 002 for 2.0mm ○ 203 for 2.3mm ○ 206 for 2.6mm

		DOCUMENT NO:	CDS-L612nn-50XX-YYZZZ-EVO	VER:	1.1
		Liquid 6 EVO Cartridge, Glass Screw-on			EFFECTIVE DATE: 1/27/2023
APPROVAL:	ECO-273	Jupiter PN(s):	See part number legend	PAGE 3 OF 4	

*XX digits denote product branding

Liquid 6 EVO, Glass Screw-on Cartridge Filling Instructions


Failure to follow these instructions may result in cartridge leakage or poor performance.

Jupiter Liquid 6 EVO, Glass Screw-on Cartridges are top-fill cartridges available in both 0.5 and 1.0 ml versions. The two versions differ only in the length of the reservoir. If you are unsure which version you have, measure the length without the mouthpiece. Refer to the drawing on page 1 to determine where to measure and which cartridge you have.

Multiple mouthpiece styles are available. All screw on in the same manner.

Filling Instructions

1. Insert a blunt tipped needle (14 ga. or smaller) into the space between the airway and the outer wall of the cartridge (see the image, below).

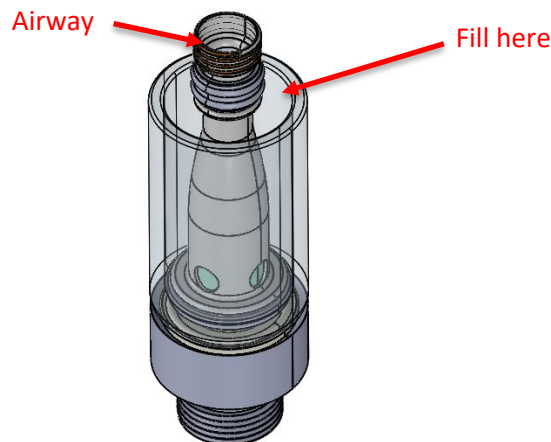


While the cartridge is oriented vertically with the threaded connector downward, fill the cartridge through the needle. Do not overfill.

Caution: Do not allow fluid to enter the airway (center tube).

2. Immediately after filling, install the mouthpiece and twist clockwise to tighten. Do not overtighten, the mouthpiece is installed correctly when the seal on the bottom of the mouthpiece is seated inside the glass housing.

Caution: Failure to install the mouthpiece within 2 minutes of filling may result in leakage.

3. Cartridges should be allowed to stand for at least 30 minutes before use. During this time, fluid is priming the atomizer. The rate that the atomizer saturates is dependent upon the viscosity of the fluid. More viscous fluids may require more time.

		DOCUMENT NO:	CDS-L612nn-50XX-YYYZZZ-EVO	VER:	1.1
		Liquid 6 EVO Cartridge, Glass Screw-on			EFFECTIVE DATE: 1/27/2023
APPROVAL:	ECO-273	Jupiter PN(s):	See part number legend	PAGE 4 OF 4	

4. If the cartridge/device is to experience a pressure change as a result of an increase in temperature or a change in elevation, the cartridge/device must be shipped with the MP facing down, allowing for the inlets to be exposed to ambient air.
5. Storage and Operation Recommendations:

Operating Temperature and Humidity	<ul style="list-style-type: none"> ○ Working Temperature: -10 °C to 60 °C ○ Operating humidity: 35% to 70%
Storage Temperature and Humidity	<ul style="list-style-type: none"> ○ Storage Temperature: 23 ± 5 °C ○ Storage Humidity: 35% to 70%